

Optical Remote Sensing with Differential Asorption Lidar (DIAL)

Part 1: Theory

Christoph Senff

CIRES, University of Colorado &
NOAA/ESRL/CSD/Atmospheric Remote Sensing Group

<http://www.esrl.noaa.gov/csd/groups/csd3/>



Guest lecture for ASEN-6365 Lidar Remote Sensing
CU Boulder

April 20, 2016


Outline

- DIAL concept
- A short history of DIAL
- DIAL equation
- Precision & accuracy of DIAL retrieval
- Dual-DIAL technique

Differential Absorption Lidar (DIAL) Concept

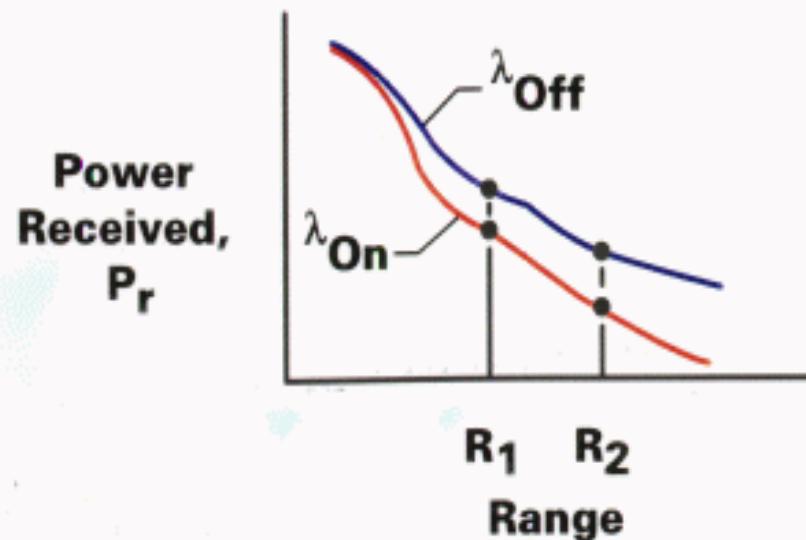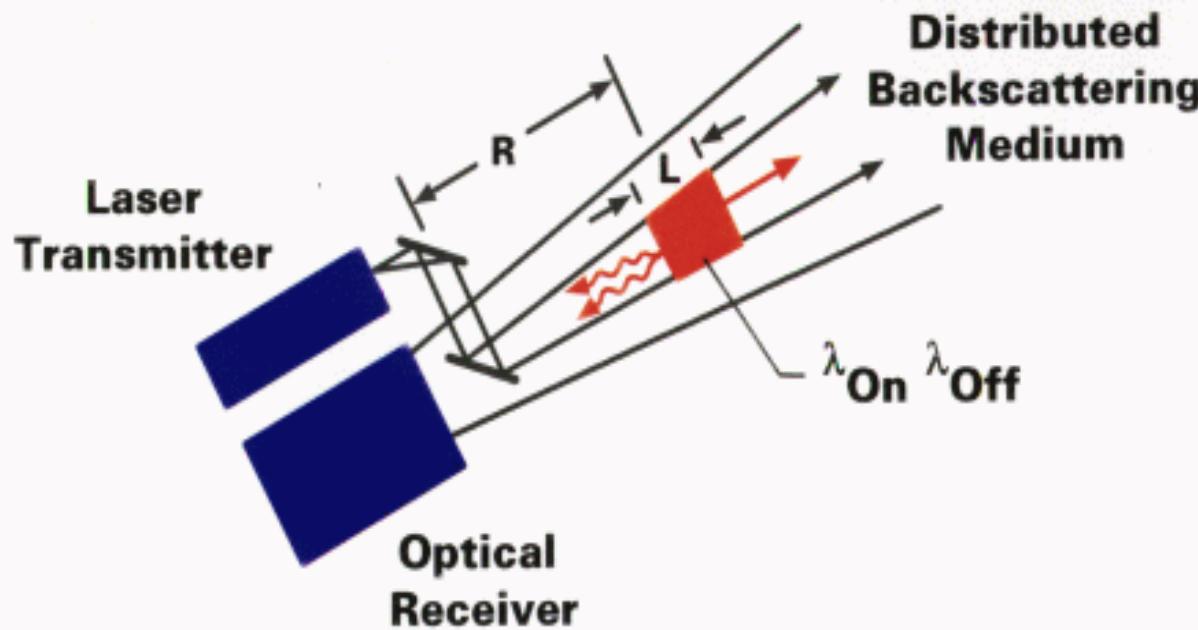

Absorption
Cross
Section

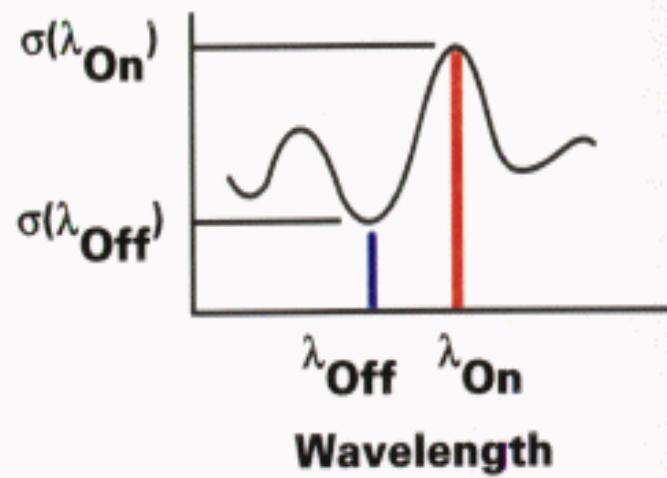

Atmospheric gases measured with DIAL

- H₂O
- O₃
- SO₂
- NO₂, NO
- NH₃
- CH₄
- CO₂
- Hg
- VOCs (Volatile Organic Compounds)
- Toluene, Benzene

First DIAL measurements

Richard M. Schotland (“The father of DIAL”)

1964 – Measured vertical profiles of water vapor by thermally tuning a ruby laser on and off the water vapor absorption line at 694.38 nm.

Only 4 years after invention of ruby laser !


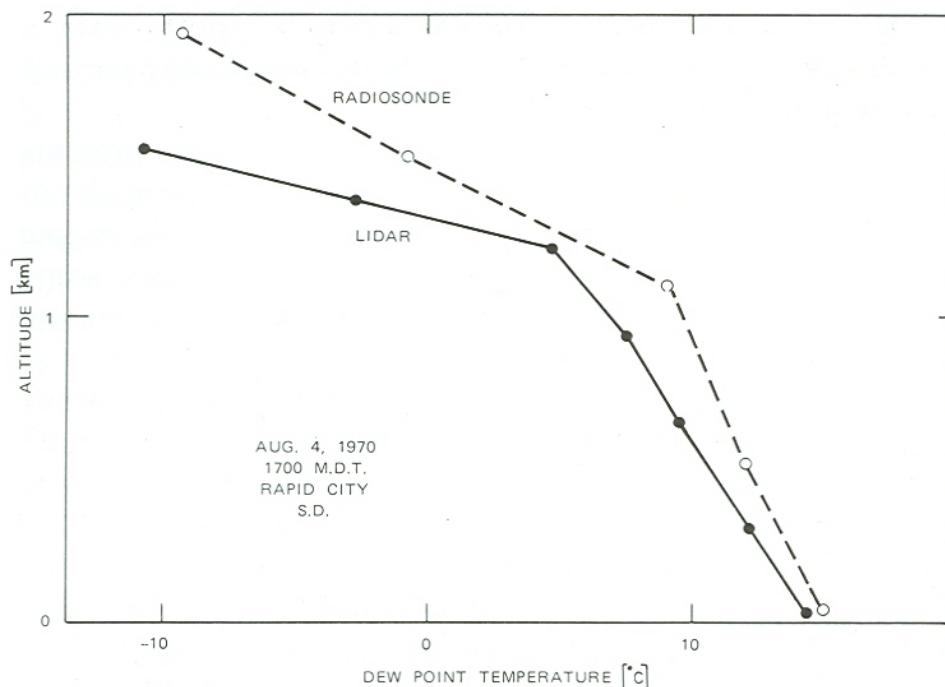


Fig. 4.20. Comparison of atmospheric water vapor vertical profiles (expressed as dew point temperature) measured by differential absorption lidar and radiosonde [4.82]

Major milestones in the history of DIAL

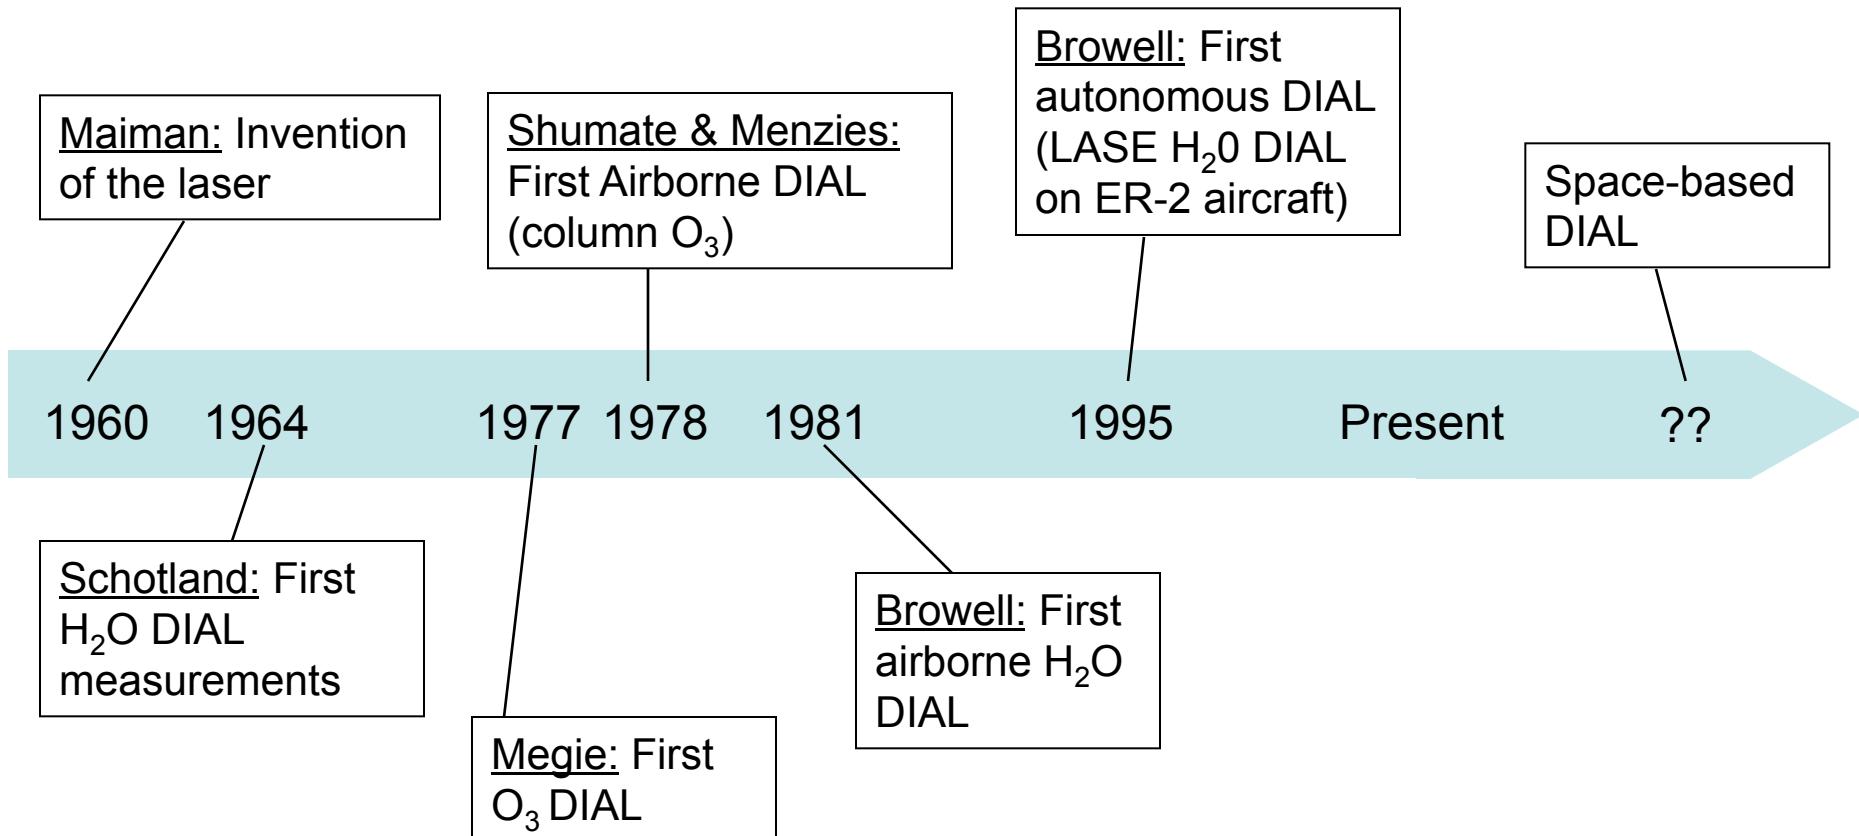

Refresher

Extinction coefficient:

$$\alpha(R), [m^{-1}]$$

Optical depth / thickness:

$$\tau(R) = \int_0^R \alpha(r) dr$$

Transmission:

$$T(R) = \exp[-\tau(R)] = \exp\left[-\int_0^R \alpha(r) dr\right]$$

DIAL equation (1)

Single scattering, elastic backscatter LIDAR equation:

$$N_S(\lambda, R) = N_L(\lambda) \left[\beta(\lambda, R) \Delta R \right] \frac{A}{R^2} \exp \left[-2 \int_0^R \alpha_{Tot}(\lambda, r) dr \right] [\eta(\lambda) G(\lambda, R)] + N_B(\lambda)$$

with $\alpha_{Tot}(\lambda, r) = \alpha(\lambda, r) + \sum_i \sigma_{mol,abs,i}(\lambda, r) n_i(r)$

Take ratio of LIDAR equations for online and offline wavelengths λ_{on} and λ_{off} :

$$\begin{aligned} \frac{N_S(\lambda_{off}, R) - N_B(\lambda_{off}, R)}{N_S(\lambda_{on}, R) - N_B(\lambda_{on}, R)} &= \frac{N_L(\lambda_{off}) \eta(\lambda_{off}) G(\lambda_{off}, R) \beta(\lambda_{off}, R)}{N_L(\lambda_{on}) \eta(\lambda_{on}) G(\lambda_{on}, R) \beta(\lambda_{on}, R)} \\ &\times \exp \left[-2 \int_0^R \alpha(\lambda_{off}, r) - \alpha(\lambda_{on}, r) dr \right] \\ &\times \exp \left[-2 \int_0^R (\sigma_C(\lambda_{off}, r) - \sigma_C(\lambda_{on}, r)) n_C(r) dr \right] \\ &\times \exp \left[-2 \int_0^R \sum_{i=1}^m [(\sigma_{X_i}(\lambda_{off}, r) - \sigma_{X_i}(\lambda_{on}, r)) n_{X_i}(r)] dr \right] \end{aligned}$$

Number density
of constituent C

DIAL equation (2)

$$n_c = \frac{1}{2\Delta\sigma_c(R)} \frac{d}{dR} \ln \left[\frac{N_s(\lambda_{off}, R) - N_b(\lambda_{off})}{N_s(\lambda_{on}, R) - N_b(\lambda_{on})} \right]$$

$$- \frac{1}{2\Delta\sigma_c(R)} \frac{d}{dR} \ln \frac{G(\lambda_{off}, R)}{G(\lambda_{on}, R)} \quad [GF]$$

$$- \frac{1}{2\Delta\sigma_c(R)} \frac{d}{dR} \ln \frac{\beta(\lambda_{off}, R)}{\beta(\lambda_{on}, R)} \quad [B]$$

$$- \frac{1}{\Delta\sigma_c(R)} [\alpha(\lambda_{on}, R) - \alpha(\lambda_{off}, R)] \quad [E]$$

$$- \frac{1}{\Delta\sigma_c(R)} \sum_{i=1}^m \Delta\sigma_{X_i}(R) n_{X_i}(R) \quad [X]$$

with $\Delta\sigma_c(R) = \sigma_c(\lambda_{on}, R) - \sigma_c(\lambda_{off}, R)$



GF = differential geometrical factor
E = differential extinction

B = differential backscatter
X = interfering constituents

How to choose an appropriate absorption line for DIAL (1)

$$N_S(\lambda_{on}, R) \propto \exp \left[-2 \int_0^R \sigma_C(\lambda_{on}, r) n_C(r) dr \right]$$

Extinction of online wavelength due to absorption by constituent C must be neither too small or too large.

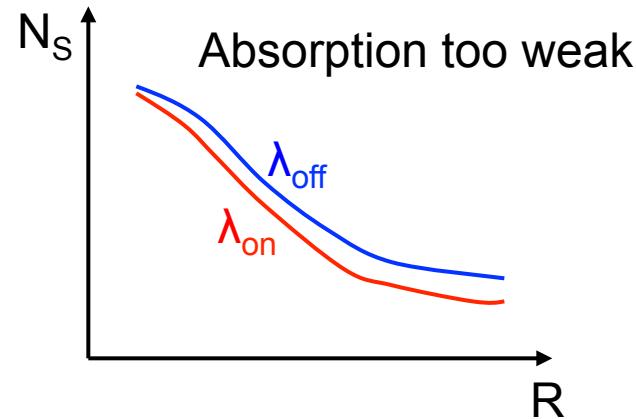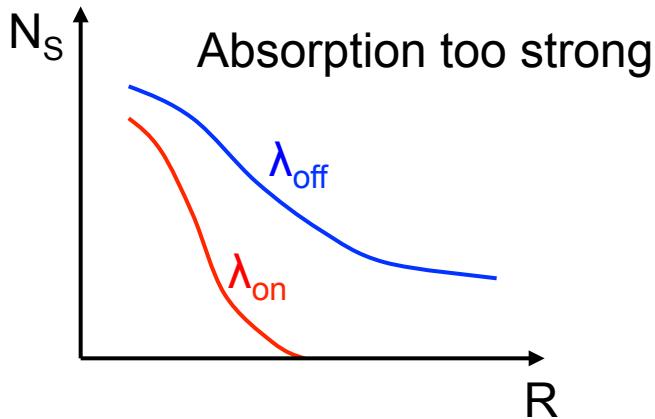

Best precision in n_C when: $\tau(\lambda_{on}, R_{\max}) = \int_0^{R_{\max}} \sigma_C(\lambda_{on}, r) n_C(r) dr = 1.1$
(Remsberg & Gordley, 1978)


How to choose an appropriate absorption line for DIAL (2)

Example: Ozone

$$\tau(\lambda_{on}, R_{\max}) = \int_0^{R_{\max}} \sigma_C(\lambda_{on}, r) n_C(r) dr = 1.1$$

For $mr_{O_3} = 80 \text{ ppbv}$ or $n_{O_3} = 2 \times 10^{18} \text{ m}^{-3}$ and $R_{\max} = 3 \text{ km}$:

$$\sigma_{O_3}(\lambda_{on}) n_{O_3} R_{\max} = 1.1 \Rightarrow \boxed{\sigma_{O_3}(\lambda_{on}) = 1.83 \times 10^{-22} \text{ m}^2}$$

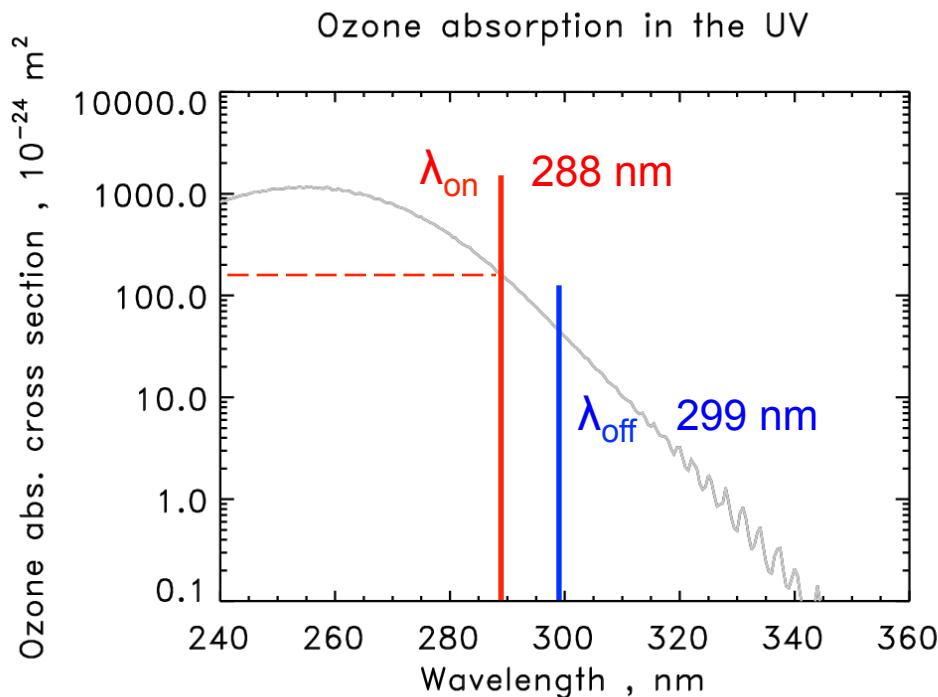

Precision of DIAL measurements

Simple “back of the envelope” calculation:

$$n_C = \frac{1}{2\Delta\sigma_C(R)\Delta R} \ln \left[\frac{N(\lambda_{off}, R + \Delta R) N(\lambda_{on}, R)}{N(\lambda_{on}, R + \Delta R) N(\lambda_{off}, R)} \right] \quad \text{with } N = N_S - N_B$$

$$\delta n_C = \frac{1}{2\Delta\sigma_C(R)\Delta R} \sqrt{\sum_{i,j} \frac{\delta^2(N(\lambda_i, R_j))}{(N(\lambda_i, R_j))^2}} \approx \frac{1}{\Delta\sigma_C \Delta R} \frac{\delta N}{N} = \frac{1}{\Delta\sigma_C \Delta R} \frac{1}{SNR} \quad \text{with } SNR = \frac{N}{\delta N}$$

$$\frac{\delta n_C}{n_C} = \frac{1}{\Delta\sigma_C n_C \Delta R SNR} = \frac{1}{\Delta\tau SNR} \quad \Rightarrow \quad SNR = \frac{1}{\Delta\tau \delta n_C / n_C}$$

Example: $\Delta\tau = 0.05$, $\delta n_C / n_C = 5\%$ \Rightarrow SNR = 400!

Even modest precision of 5% requires high SNR. SNR can be increased by averaging on/offline signals time- and range-wise.

Poisson statistics: $\delta N = N^{0.5} \Rightarrow SNR = N^{0.5}$

Since $N \propto \Delta t \Delta R$, $SNR \propto \Delta t^{0.5} \Delta R^{0.5}$ and $\delta n_C \propto \Delta t^{-0.5} \Delta R^{-1.5}$

Accuracy of DIAL measurements (1)

$$\begin{aligned} n_C = & \frac{1}{2\Delta\sigma_C(R)} \frac{d}{dR} \ln \left[\frac{N_S(\lambda_{off}, R) - N_B(\lambda_{off})}{N_S(\lambda_{on}, R) - N_B(\lambda_{on})} \right] \\ & - \frac{1}{2\Delta\sigma_C(R)} \frac{d}{dR} \ln \frac{G(\lambda_{off}, R)}{G(\lambda_{on}, R)} \quad [GF] \\ & - \frac{1}{2\Delta\sigma_C(R)} \frac{d}{dR} \ln \frac{\beta(\lambda_{off}, R)}{\beta(\lambda_{on}, R)} \quad [B] \\ & - \frac{1}{\Delta\sigma_C(R)} [\alpha(\lambda_{on}, R) - \alpha(\lambda_{off}, R)] \quad [E] \\ & - \frac{1}{\Delta\sigma_C(R)} \sum_{i=1}^m \Delta\sigma_{X_i}(R) n_{X_i}(R) \quad [X] \end{aligned}$$


Accuracy affected by:

- How well is absorption cross section known?
- Improper correction of signal offsets, e.g. background light
- Geometrical factor different for λ_{on} and λ_{off}
- Differential backscatter & extinction not properly corrected
- Interfering species not taken into account

Accuracy of DIAL measurements (2)

Differential geometrical factor:

$$-\frac{1}{2\Delta\sigma_c(R)} \frac{d}{dR} \ln \frac{G(\lambda_{off}, R)}{G(\lambda_{on}, R)} \quad [GF]$$

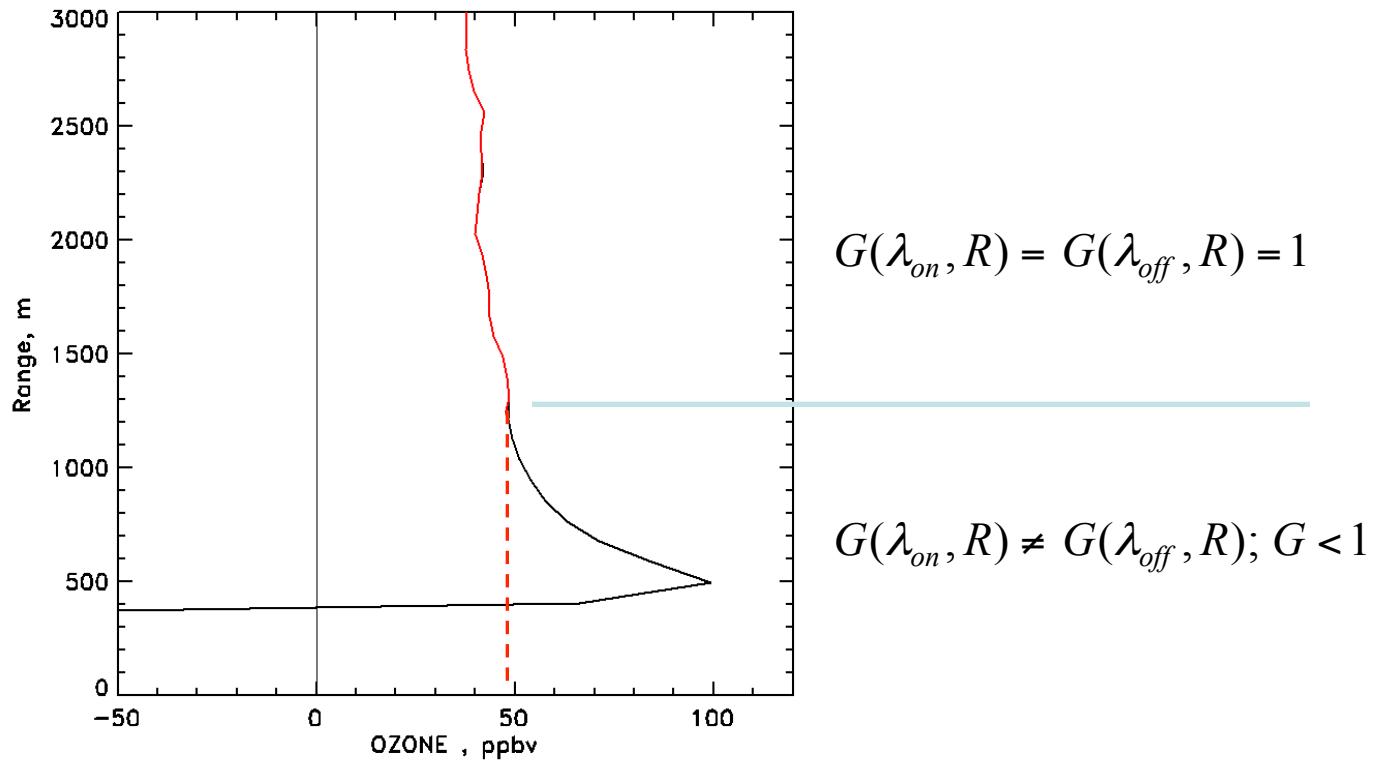

Effect of differential geometrical
factor on O₃ retrieval


Accuracy of DIAL measurements (3)

Differential backscatter & extinction:

$$-\frac{1}{2\Delta\sigma_c(R)} \frac{d}{dR} \ln \frac{\beta(\lambda_{off}, R)}{\beta(\lambda_{on}, R)} \quad [B]$$

$$-\frac{1}{\Delta\sigma_c(R)} [\alpha(\lambda_{on}, R) - \alpha(\lambda_{off}, R)] \quad [E]$$



$$\beta = \beta_{Rayleigh} + \beta_{Aerosol}, \quad \alpha = \alpha_{Rayleigh} + \alpha_{Aerosol}$$

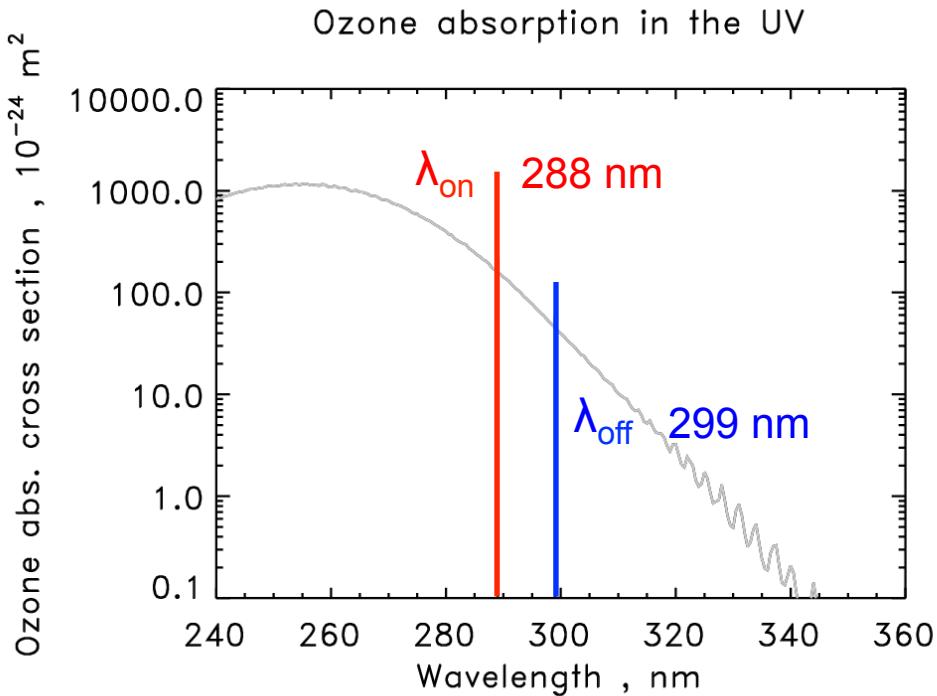

➤ For ozone DIAL retrieval, backscatter and extinction correction is necessary due to large $\Delta\lambda$.


➤ $\beta_{Aerosol}$ and $\alpha_{Aerosol}$ have to be determined from offline signal data and wavelength dependence of β and α have to be guessed.

Accuracy of DIAL measurements (4)

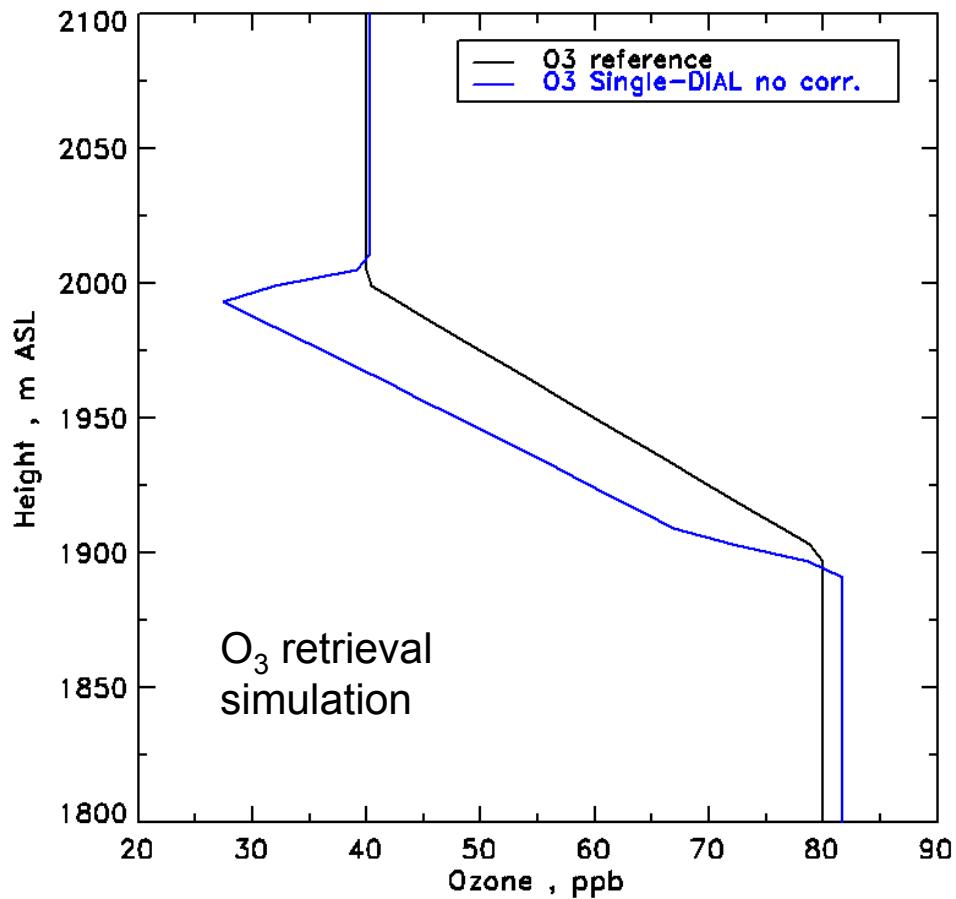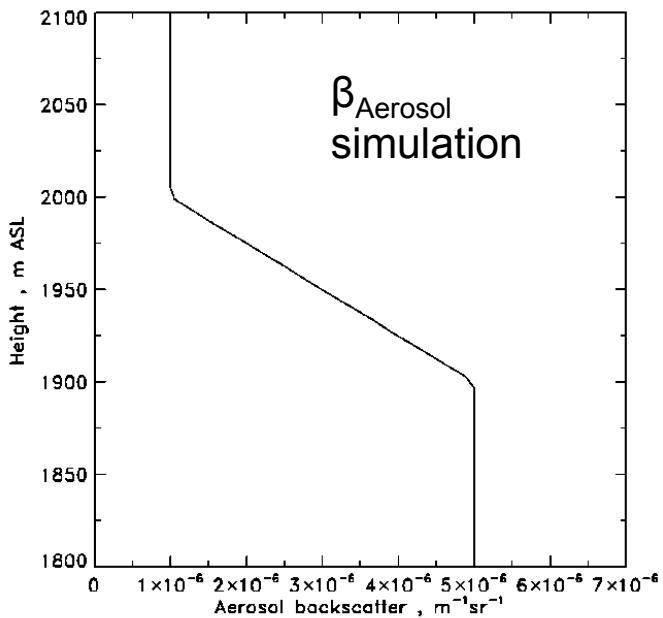

Wrong assumptions about aerosol parameters can introduce significant errors in O₃ retrieval !

Dual-DIAL concept

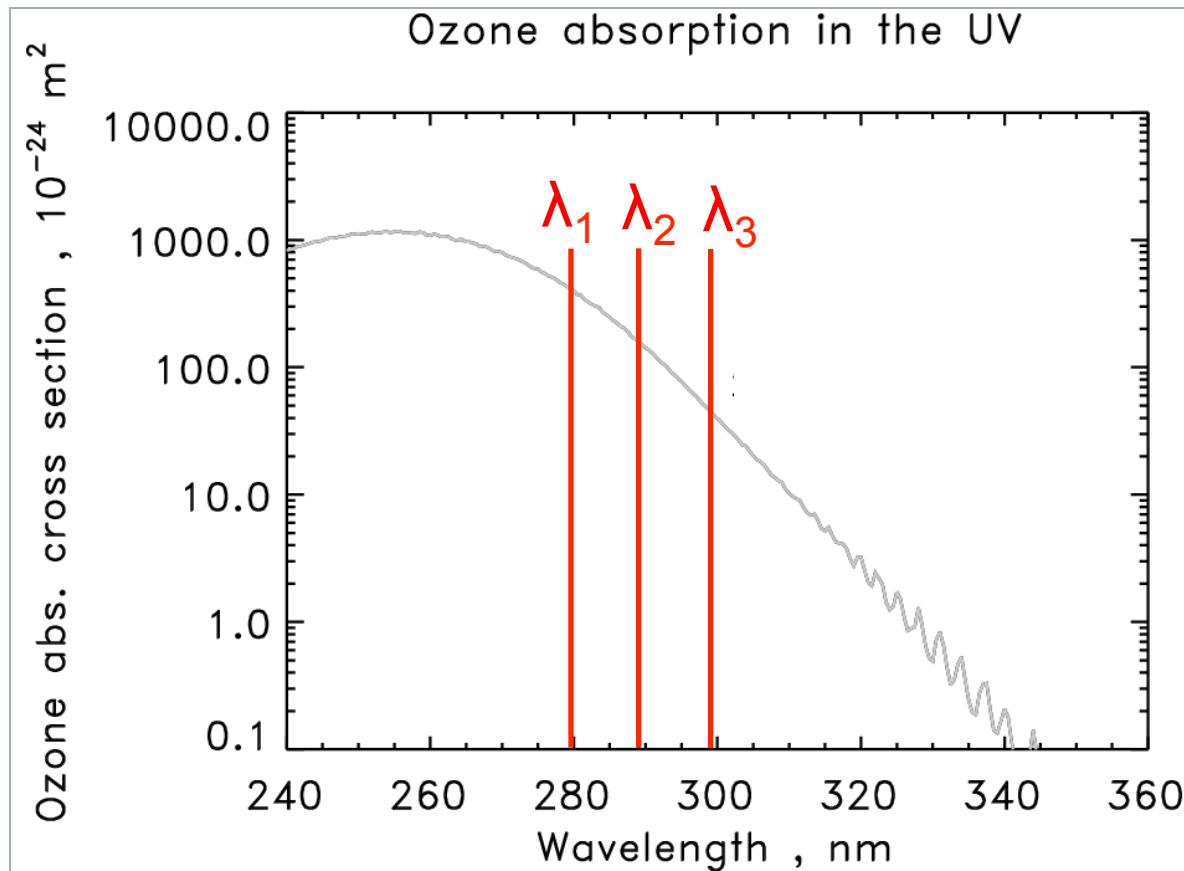

2 DIAL wavelength pairs: λ_1 / λ_2 and λ_2 / λ_3

Dual-DIAL minimizes aerosol interference (1)


$$n_C = \frac{1}{2\delta\sigma_C(R)} \frac{d}{dR} \left[\ln \frac{N_S^*(\lambda_{off1}, R)}{N_S^*(\lambda_{on1}, R)} - C \ln \frac{N_S^*(\lambda_{off2}, R)}{N_S^*(\lambda_{on2}, R)} \right]$$
$$- \frac{1}{2\delta\sigma_C(R)} \frac{d}{dR} \left[\ln \frac{\beta(\lambda_{off1}, R)}{\beta(\lambda_{on1}, R)} - C \ln \frac{\beta(\lambda_{off2}, R)}{\beta(\lambda_{on2}, R)} \right] \quad [B']$$
$$- \frac{1}{\delta\sigma_C(R)} [\alpha(\lambda_{on1}, R) - \alpha(\lambda_{off1}, R) - C(\alpha(\lambda_{on2}, R) - \alpha(\lambda_{off2}, R))] \quad [E']$$

with $\delta\sigma_C(R) = \Delta\sigma_{C1} - C \Delta\sigma_{C2}$, DIAL pair 1: $\lambda_{on1} / \lambda_{off1}$, DIAL pair 2: $\lambda_{on2} / \lambda_{off2}$

$$B' = E' \approx 0 \quad \text{for} \quad C = \frac{\lambda_{on1} - \lambda_{off1}}{\lambda_{on2} - \lambda_{off2}}$$

- No correction of differential aerosol effects needed and residual errors are small.
- However, precision of DIAL retrieval is degraded.

Dual-DIAL minimizes aerosol interference (2)

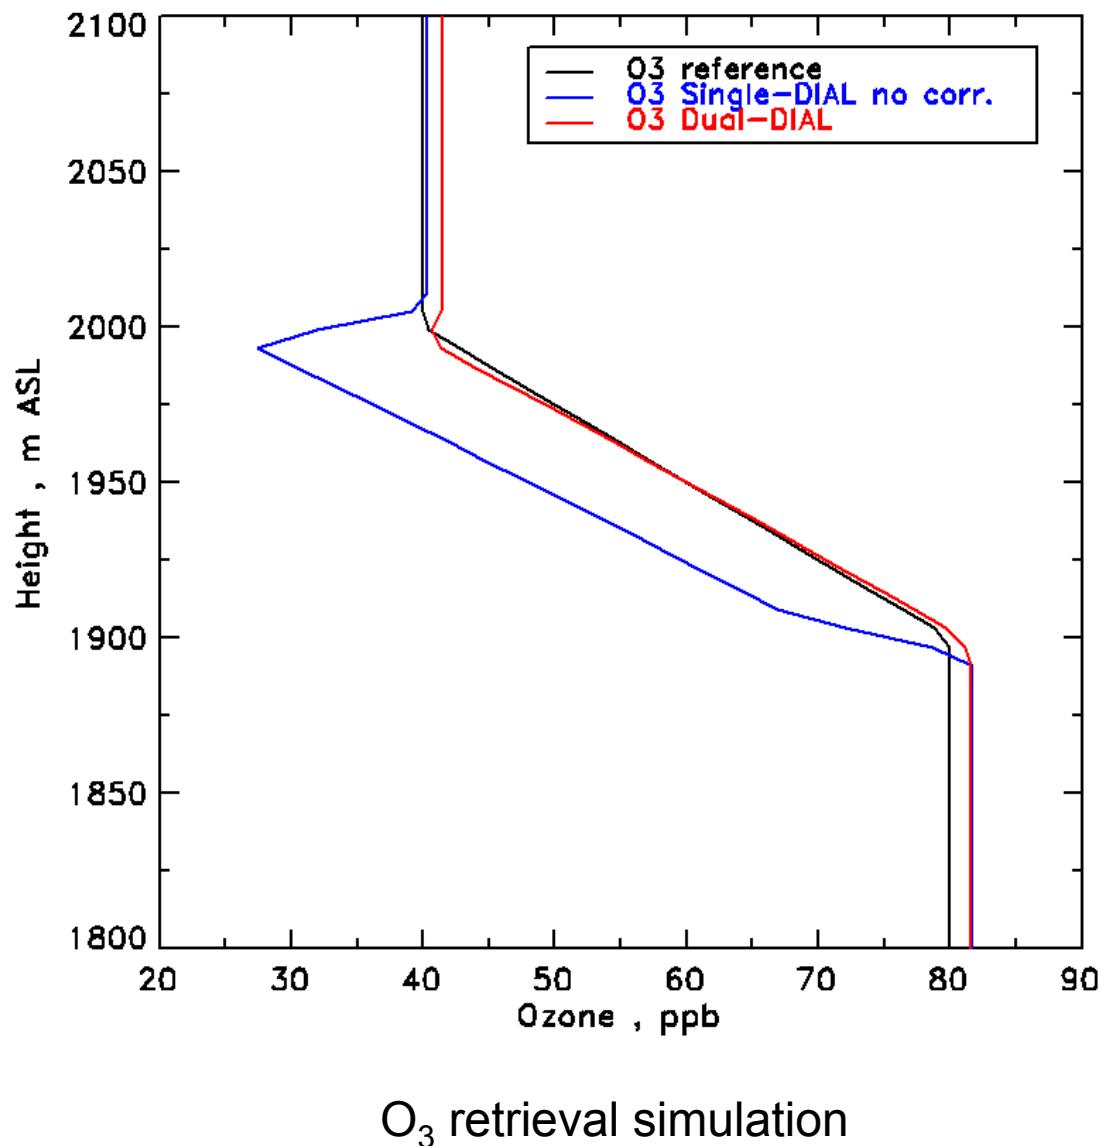

Selected References

DIAL history (slides 5 - 6)

- Schotland, R. M., 1974: Errors in the Lidar Measurement of Atmospheric Gases by Differential Absorption, *J. Appl. Meteorol.*, **13**, 71-77.
- Shumate, M. S., R. T. Menzies, W. B. Grant, and D. S. McDougal, 1981: Laser Absorption Spectrometer: Remote Measurement of Tropospheric Ozone, *Appl. Opt.*, **20**, 545-553.
- Pelon, J. and G. Megie, 1982: Ozone Monitoring in the Troposphere and Lower Stratosphere: Evaluation and Operation of a Ground-Based Lidar Station, *J. Geophys. Res.*, **87**, 4947-4955.
- Megie, G. J., G. Ancellet, and J. Pelon, 1985: Lidar Measurements of Ozone Vertical Profiles, *Appl. Opt.*, **24**, 3454-3463.
- Browell, E. V., S. Ismail, W. B. Grant, 1998: Differential Absorption Lidar (DIAL) Measurements from Air and Space, *Appl. Phys. B*, **67**, 399 – 410.
- Ismail, S., E. V. Browell, R. A. Ferrare, S. A. Kooi, M. B. Clayton, V. G. Brackett and P. B. Russell, 2000: LASE Measurements of Aerosol and Water Vapor Profiles During TARFOX, *J. Geophys. Res.*, **105**, D8, 9903-9916.

How to choose a DIAL absorption line? (slides 10 - 11)

- Remsberg, E. E. and L. L. Gordley, 1978: Analysis of Differential Absorption Lidar from the Space Shuttle, *Appl. Opt.*, **17**, 624-630.

Aerosol correction & DUAL-DIAL (slides 15 - 19)

- Browell, E. V., S. Ismail, and S. T. Shipley, 1985: Ultraviolet DIAL measurements of O₃ profiles in regions of spatially inhomogeneous aerosols, *Appl. Opt.*, **24**, 2827-2836.
- Wang, Z., H. Nakane, H. Hu, and J. Zhou, 1997: Three-Wavelength Dual Differential Absorption Lidar Method for Stratospheric Ozone Measurements in the Presence of Volcanic Aerosols, *Appl. Opt.*, **36**, 1245-1252.